



## Certificate of Analysis

Date:	2025-05-05 11:57:20 -04:00	Cultivar:	
Serial:	LL030645	Moisture:	0.0%
LightLab	BW-LABS	Col Tests Remaining:	6
Operator:		CoA Revision:	0
Sample ID:		Calibration Exp:	2026-03-21
Method:	LightLab HPLC	Product:	Strawberry D8 25 mg
Test Type:	Gummy- Advanced	SKU:	Daiana
Weight / Volume:	0.55 g	Batch:	D8SIG1185
Solvent:	40 ml		
Temperature:	27.6 °C		
Notes:			


### Cannabinoid Profile

Analyte	Per 7.200 g Serving (mg)	Per 1.0 Pieces(mg)	%	LOQ
THC-A	ND	ND	ND	0.012
Δ9-THC	ND	ND	ND	0.012
CBD-A	ND	ND	ND	0.012
CBG-A	ND	ND	ND	0.012
CBD/CBG	1.7	1.7	0.024	0.012
CBN-A	ND	ND	ND	0.012
CBN	ND	ND	ND	0.012
CBC-A	ND	ND	ND	0.012
CBC	ND	ND	ND	0.012
Δ8-THC*	25.4	25.4	0.35	0.094
Δ10-THC	ND	ND	ND	0.012
THCV-A	1.2	1.2	0.016	0.012
THCV	ND	ND	ND	0.012
Terpenes			Low	
<b>Total THC</b>	<b>ND</b>	<b>ND</b>	<b>ND</b>	
<b>Total Cannabinoids</b>	<b>28.2</b>	<b>28.2</b>	<b>0.39</b>	

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC =  $(0.877 \times \text{THC-A}) + \Delta 9\text{-THC}$ ; Total CBD =  $(0.877 \times \text{CBD-A}) + \text{CBD}$ . \* Δ8THC has lower precision and higher detection limit than other cannabinoids.

## Chromatogram

---

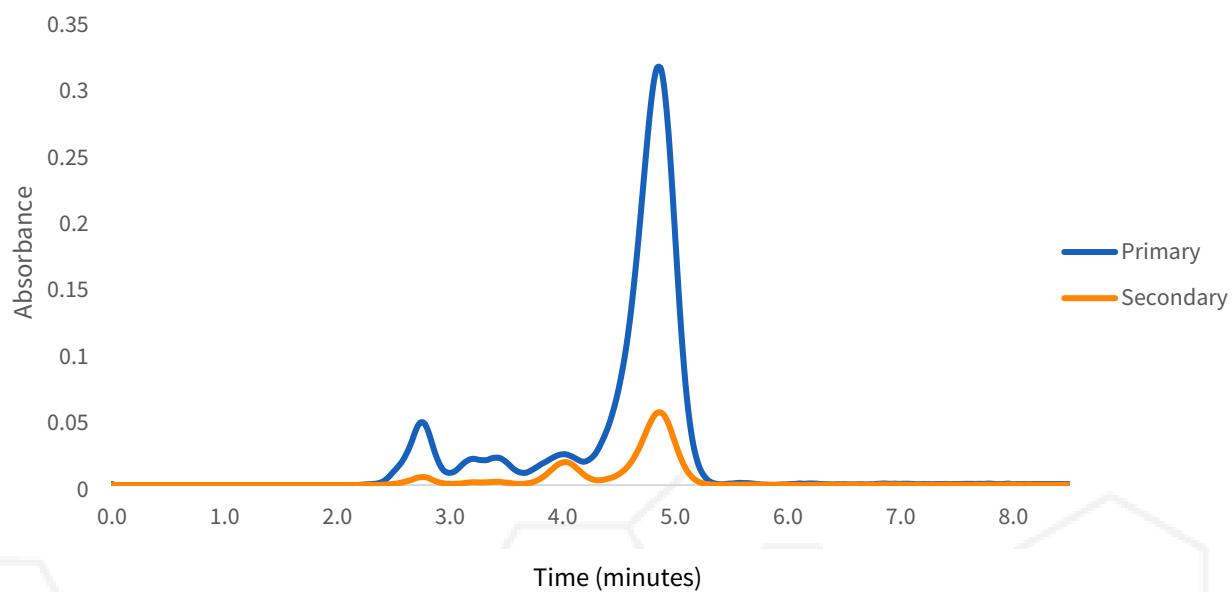

## Sample Images

---



## Change History

---

Date	User	Action
2025-05-05 11:57:20 -04:00		Test Recorded
2025-05-16 12:38:07 -04:00	DA	Added an image
2025-05-16 12:40:29 -04:00	DA	Changed EdblProduct from "D8" to "Strawberry D8 25 mg". Changed EdblName from "" to "Daiana". Changed Batch from "" to "D8SIG1185".
2025-05-16 12:40:31 -04:00		Generated a CoA (revision 0)



5/5/2025



Scan for Authenticity

Approved

Date

The signatory confirms that the Operator has performed the sample preparation according to the LightLab User's Guide. This report is for quality assurance purposes only. These results relate only to the sample included on this report. Orange Photonics makes no claims as to the efficacy, safety, or risks associated with any detected or non-detected level of any compounds reported herein. Orange Photonics makes no claims regarding the adherence to sample preparation guidelines, by the operator, as outlined in the LightLab User's Guide.

